

Attribution-NonCommercial-NoDerivs 3.0 Unported (CC BY-NC-ND 3.0)

<https://creativecommons.org/licenses/by-nc-nd/3.0/>

Access to this work was provided by the University of Maryland, Baltimore County (UMBC) ScholarWorks@UMBC digital repository on the Maryland Shared Open Access (MD-SOAR) platform.

**Please provide feedback**

Please support the ScholarWorks@UMBC repository by emailing [scholarworks-group@umbc.edu](mailto:scholarworks-group@umbc.edu) and telling us what having access to this work means to you and why it's important to you. Thank you.

## Communication

Pradeep Kumar Badiya<sup>a</sup>, Tejkiran Pindi Jayakumar<sup>a</sup>, Venkatesh Srinivasan  
and Sai Sathish Ramamurthy\*

# Spacer layer engineering for ultrasensitive Hg(II) detection on surface plasmon-coupled emission platform

DOI 10.1515/ntrev-2017-0124

Received February 17, 2017; accepted April 25, 2017; previously published online June 15, 2017

**Abstract:** In this work, we demonstrate for the first time the ultrasensitive detection of Hg<sup>2+</sup> ions with femtomolar sensitivity in water samples with the use of the surface plasmon-coupled emission (SPCE) platform. The use of portable network diagnostic tools for water security and integrated water shed management is a topic of recent research interest. In this context, the current study explores Hg<sup>2+</sup> monitoring using a rhodamine-6G (Rh6G) derivative bearing a monothiospirolactone mounted onto a SPCE substrate. Thus far, the limit of detection for mercury ions by the conventional fluorescence technique has been 0.15 nM. However, we have achieved 1 fM Hg<sup>2+</sup> detection using silver nanoparticle-based spacer layer engineering on an SPCE sensor chip. Using this technology, a field device can be fabricated for rapid, ultrasensitive, multi-analyte detection (of contaminants) in water samples.

**Keywords:** fluorescence enhancements; mercury sensing; silver nanoparticles; spacer engineering; surface plasmon-coupled emission.

## 1 Introduction

Access to potable drinking water, essential for human sustenance, is a foremost concern in the 21st century. This

situation has risen as a large extent of water resources is affected by geogenic and anthropogenic sources. Heavy metal ions in this context are particularly long-term hazardous toxicants on account of their high toxicity, retention, and accumulation in the human body. Their influence on the environment and nature is disparaging [1–3]. Among the transition and heavy metal ions, mercury contamination is of research interest due to its widespread contamination and its origin form: mining [4], waste incineration, fossil fuel combustion [5], Portland cement manufacturing, volcanic eruptions [6], and oceanic emissions [7], to name a few. Mercury is employed in several applications that include batteries, fluorescent light bulbs, compact fluorescents, thermometers, thermostats, amalgam in dental fillings, thimerosal in vaccines, and automotive switches. Mercury is known for its severe genotoxic, immunotoxic, and neurotoxic effects [8]. Organic mercury, especially, is highly soluble in water and passes easily through the biological membranes, causing damage to the central nervous and endocrine systems, and is found to be more toxic than the inorganic mercury salts [9]. This necessitates rapid and sensitive detection of mercury ions with a specific focus on data collection networks for an integrated water management approach.

There are different well-established protocols for mercury estimation: inductively coupled plasma spectroscopy, atomic absorption spectroscopy, molecular absorption spectroscopy, and electro-analytical techniques, to name a few [10]. However, these techniques involve significant sample preparation time scales, need cumbersome equipment, require trained personnel, and are financially heavy and not suitable for a resource-limited setting. In this regard, fluorescence spectroscopy offers an alternative and rapid method for metal ion screening. A variety of fluorescent chemosensors have been developed based on rhodamine derivatives [11–15], fluorescein derivatives [16–18], NO<sub>2</sub>S<sub>2</sub>-donor macrocycles [19], naphthalimide [20], oligonucleotides [21], genetically engineered cells [22], nanomaterials [23], foldamers [24], and DNAzymes

\*Pradeep Kumar Badiya and Tejkiran Pindi Jayakumar: These authors contributed equally to this study.

\*Corresponding author: Sai Sathish Ramamurthy, Plasmonics Laboratory, Department of Chemistry, Sri Sathya Sai Institute of Higher Learning, Prasanthi Nilayam, Anantapur, Andhra Pradesh 515134, India, Phone: +91-8790314405, e-mail: rsaisathish@sssihl.edu.in

Pradeep Kumar Badiya, Tejkiran Pindi Jayakumar and Venkatesh Srinivasan: Plasmonics Laboratory, Department of Chemistry, Sri Sathya Sai Institute of Higher Learning, Prasanthi Nilayam, Anantapur, Andhra Pradesh 515134, India

[25]. Among the abovementioned chemosensors, rhodamine-based fluorescence detection has been preferred due to the well-understood photochemical processes, low cost, long-wavelength (>500 nm) absorption or emission, high molar absorption coefficient, and quantum yield of these derivatives. These optical sensors have an interesting metal ion response, a turn “on/off” behavior. In the absence of the metal ions, the molecule prefers the spiro-lactam ring closed, with little or no absorption in the visible region. However, in the presence of the metal ions, chelation occurs, resulting in ring opening and simultaneous creation of a highly absorbing, fluorescent complex.

Nevertheless, there are limitations in the conventional fluorescence technique, including low collection efficiency (<1%) arising due to its isotropic emission, interference by scattered light, photobleaching of the fluorophore, and a congested fluorescence emission spectrum on account of spectral broadening. In this context, surface plasmon-coupled emission (SPCE), as a technique that alters the behavior of excited fluorophores in proximity to nanometer-thick metal films, has gained importance. SPCE is a near-field phenomenon that results when a few-nanometer-thick layer containing radiating dipoles is positioned above a thin silver film (50 nm) that couples >50% of the fluorescence (1% in conventional fluorescence platform) into the surface plasmons. Due to the outcoupling conditions of the surface plasmons (electronic oscillations on metal thin films), the light passing through a transparent prism is polarized directional emission with significant background suppression [26, 27]. To augment the coupling of fluorescence, we have introduced an additional spacer layer sandwiched between the fluorophore and the silver thin film. Our spacer layer engineering has presented significant enhancements (in excess of thousand fold) in SPCE, with the use of hybrid spacers that include low-dimensional carbons, biomaterials, semiconductor nanoparticles, noble metal nanoparticles, and their composites [28–31]. These novel SPCE substrates have found convergent application in monitoring of LpPLA<sub>2</sub> (coronary heart disease marker at picomolar concentration), organic dye systems (at femtomolar concentration), and dopamine and DNA (at attomolar concentration) [28–34]. In the present study, we extend the capability of this platform for ultrasensitive monitoring of mercury ions in water.

## 2 Materials and methods

Rhodamine-6G (Rh6G) and polyvinyl alcohol (PVA) were purchased from Sigma Aldrich, St. Louis, MO, USA. HgCl<sub>2</sub>, HPLC-grade acetonitrile, and tetrahydrofuran (THF) were

procured from Merck Specialties Private Limited, Mumbai, Maharashtra, India. Thiourea, phosphorus oxychloride, and 1,2-dichloroethane were sourced from SD Fine Chemicals, Mumbai, Maharashtra, India. Silver nanoparticles (AgNPs, 20 nm) were acquired from BBI Solutions, Redding, CA, USA. Pyrex slides coated with a 50-nm-thick silver thin film and a 5-nm-thick silica top layer were purchased from EMF Corp., Ithaca, NY, USA. Millipore water (18 MΩ cm<sup>-1</sup>) was used to prepare all the solutions for the current study.


### 2.1 Synthesis of the Rh6G derivative (Rh6G D)

A two-step preparation of the rhodamine derivative was carried out, as reported earlier [14]. In the first step, Rh6G (3 g, 6.3 mmol) was added to a solution of NaOH (4.8 g, 0.12 mol) in a mixture of ethanol (30 ml) and water (60 ml). The solution was refluxed for 12 h and then cooled to room temperature, followed by the evaporation of the ethanol in vacuum. The pH of the solution was adjusted to 6–7 using 2 M HCl. The precipitate obtained was filtered, washed several times with water, and dried to obtain A.

In the second step, to the stirred solution of A (2 g, 4.8 mmol) in 1,2-dichloroethane, 3 ml phosphorus oxychloride was added dropwise. The reaction mixture was refluxed for 4 h, followed by cooling and evaporation in vacuum. The crude acid chloride was then dissolved in 6 ml THF and added dropwise to a solution containing thiourea (1.52 g, 20 mmol), 12 ml triethyl amine in a mixture of 50 ml THF and 10 ml water at room temperature. The solvent was removed under reduced pressure after stirring the solution overnight. Water (50 ml) was added, and the precipitate formed was filtered, washed with water several times, and dried to obtain Rh6G D. The reaction scheme is presented in the Figure 1A and B illustrates the SPCE instrumental setup showing the following: A – 532 nm laser for excitation, B – aperture for adjustment, C – silver slide for mounting the sample, D – hemi-cylindrical prism, E – filter, and F – detector.

### 2.2 Fabrication of the SPCE substrate

An aqueous 40 mM stock solution of HgCl<sub>2</sub> was prepared initially. Aqueous solutions of various concentrations ranging from 400 nM to 4 fM were prepared by serial dilution. A 2% PVA aqueous solution was prepared by mild heating, and a 4 mM solution of Rh6G D was made using acetonitrile. Rh6G D (1 mM) in 1% PVA was equilibrated with different concentrations of mercury ions and

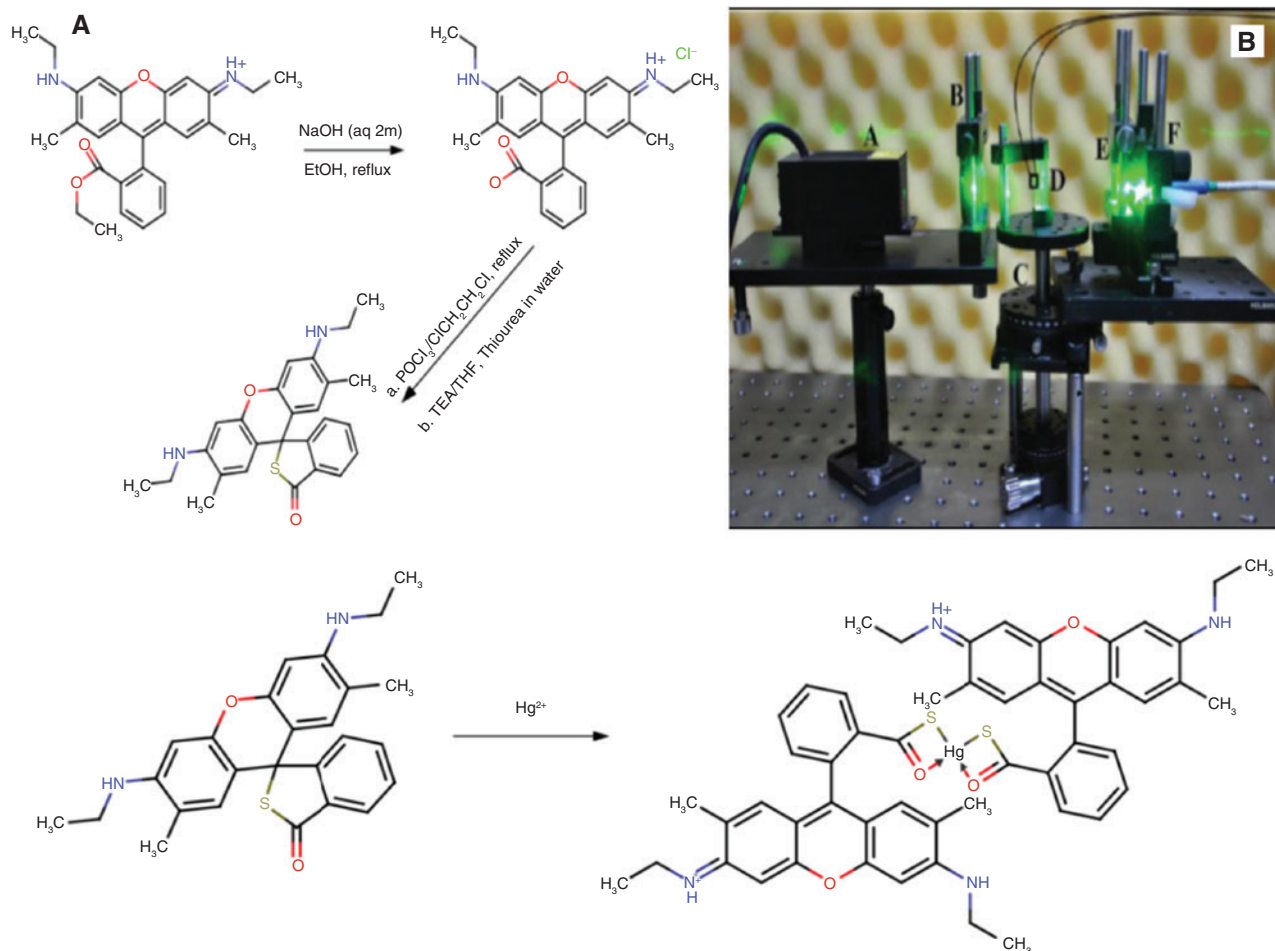


**Figure 1:** (A) Reaction scheme for the preparation of Rh6G D; (B) SPCE instrumental setup (A – 532 nm laser, B – aperture, C – silver slide, D – hemi-cylindrical prism, E – filter, and F – detector); and (C) Rh6G D-Hg<sup>2+</sup> complex formation.


then spin coated onto the SPCE substrate. Spin coating was carried out on the silver slide at 3000 rpm for 60 s to obtain a 30-nm polymer overcoat. These substrates were attached to a BK7 hemi-cylindrical prism using an index matching fluid and mounted onto a rotating stage. The slides using AgNPs were also fabricated in the same manner, with a layer of AgNPs in PVA spin coated prior to spin coating the fluorophore.

### 3 Results and discussion

On the addition of Rh6G D to a solution containing Hg<sup>2+</sup> ions, chelation of Hg<sup>2+</sup> with the sulfur and oxygen atoms results in ring opening of the monothiospirolactone (in the derivative). The formation of the complex is due to the inherent affinity of Hg<sup>2+</sup> toward sulfur [14]. The Rh6G D forms a 2:1 stoichiometric complex with the mercury ions,

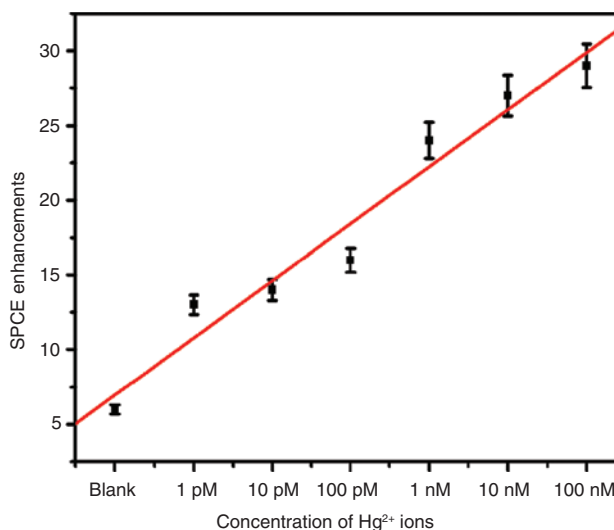

**Figure 2:** Concentration plot indicating SPCE enhancements for different Hg<sup>2+</sup> concentrations.

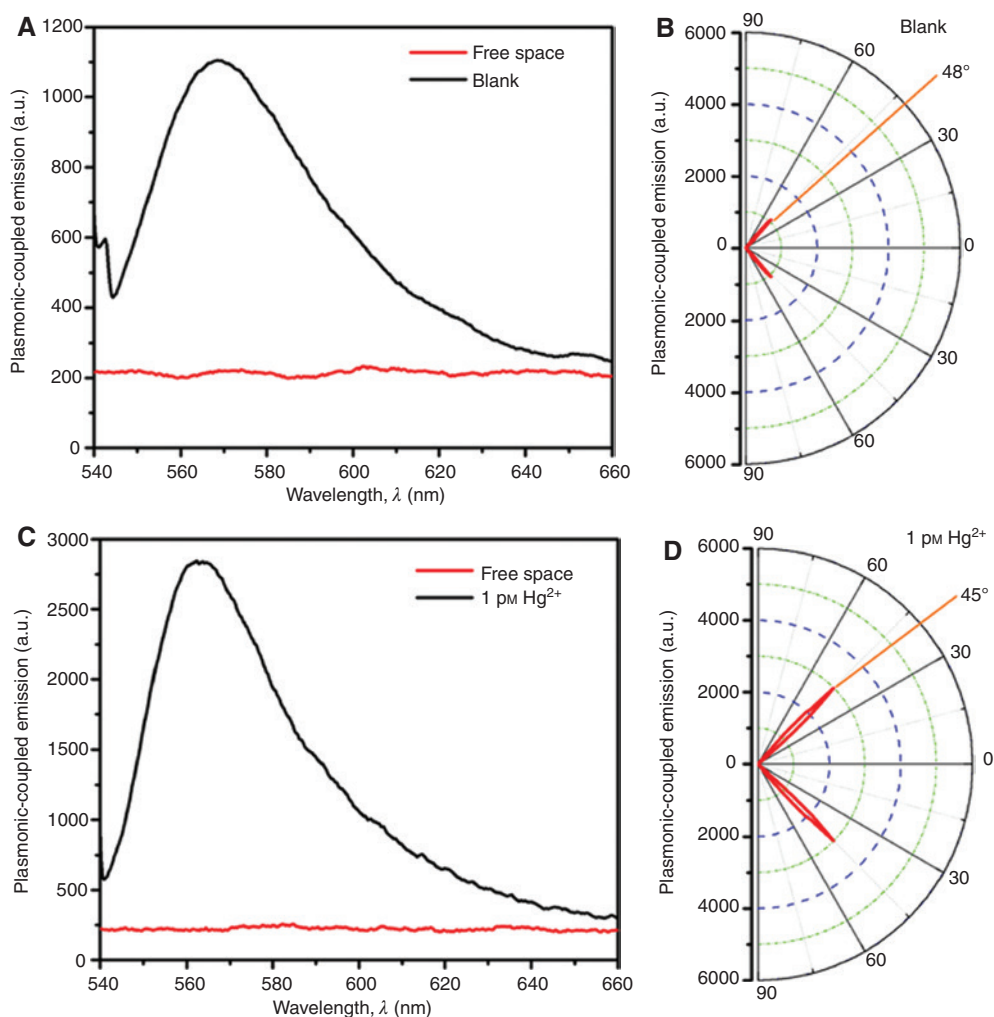

**Figure 3:** (A) SPCE and FS intensity of Rh6G D in the absence of  $\text{Hg}^{2+}$ ; (C) SPCE and FS intensity of Rh6G D in the presence of  $\text{Hg}^{2+}$ ; and SPCE radial plots for (B) blank and (D) 1  $\mu\text{M}$   $\text{Hg}^{2+}$ .


as depicted in Figure 1C. The Rh6G D in the presence of the  $\text{Hg}^{2+}$  ions consequently behaves as a fluorescent turn-on switch.

In a recent report, a limit of detection (LOD) of 0.15 nM  $\text{Hg}^{2+}$  ions was achieved using Rh6G D in conventional fluorescence spectroscopy [35]. However, in this study,

**Table 1:** SPCE enhancements and angularity obtained for different  $\text{Hg}^{2+}$  concentrations using Rh6G D (with and without an AgNP spacer layer).

Concentration of $\text{Hg}^{2+}$	Without AgNP spacer layer		With AgNP spacer layer	
	SPCE enhancements	Angle ( $^\circ$ )	SPCE enhancements	Angle ( $^\circ$ )
100 nM	35	45	82	55
10 nM	28	46	67	55
1 nM	26	44	64	56
100 $\mu\text{M}$	17	45	60	55
10 $\mu\text{M}$	15	46	58	55
1 $\mu\text{M}$	13	45	56	56
100 fM	—	—	45	55
10 fM	—	—	34	54
1 fM	—	—	20	55
Blank	6	48	10	50




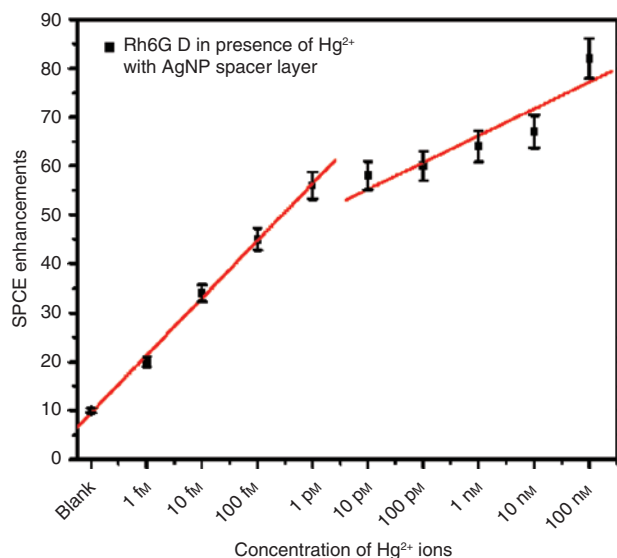

**Figure 4:** Concentration plot indicating AgNP spacer layer-dependent SPCE enhancements for different Hg<sup>2+</sup> concentrations.

the LOD of 1 fM Hg<sup>2+</sup> ions was achieved, highlighting the sensitivity of the SPCE platform in comparison with the conventional fluorescence technique. Two experiments were carried out as part of this study. Firstly, the detection of Hg<sup>2+</sup> ions was studied using plain Rh6G D encapsulated in the polymer matrix, followed by the use of AgNPs as the spacer layer on the SPCE sensor chip for augmented SPCE enhancements.

In the first set of experiments, Hg<sup>2+</sup> ions at 1 pM were detected with a 13-fold enhancement of fluorescence over the free space (FS) emission. A 35-fold enhancement was achieved in the presence of 100 nM concentration of Hg<sup>2+</sup> over its FS emission. The fluorescence of Rh6G D in the absence of Hg<sup>2+</sup> was about 6-fold higher compared to FS. Figure 2 presents the SPCE enhancements achieved for different concentrations of Hg<sup>2+</sup> ranging from 100 nM to 1 pM. The fluorescence spectrum of Rh6G D in the absence of Hg<sup>2+</sup> (blank) along with its FS spectrum have been plotted in Figure 3A, and B shows the SPCE angularity plot with

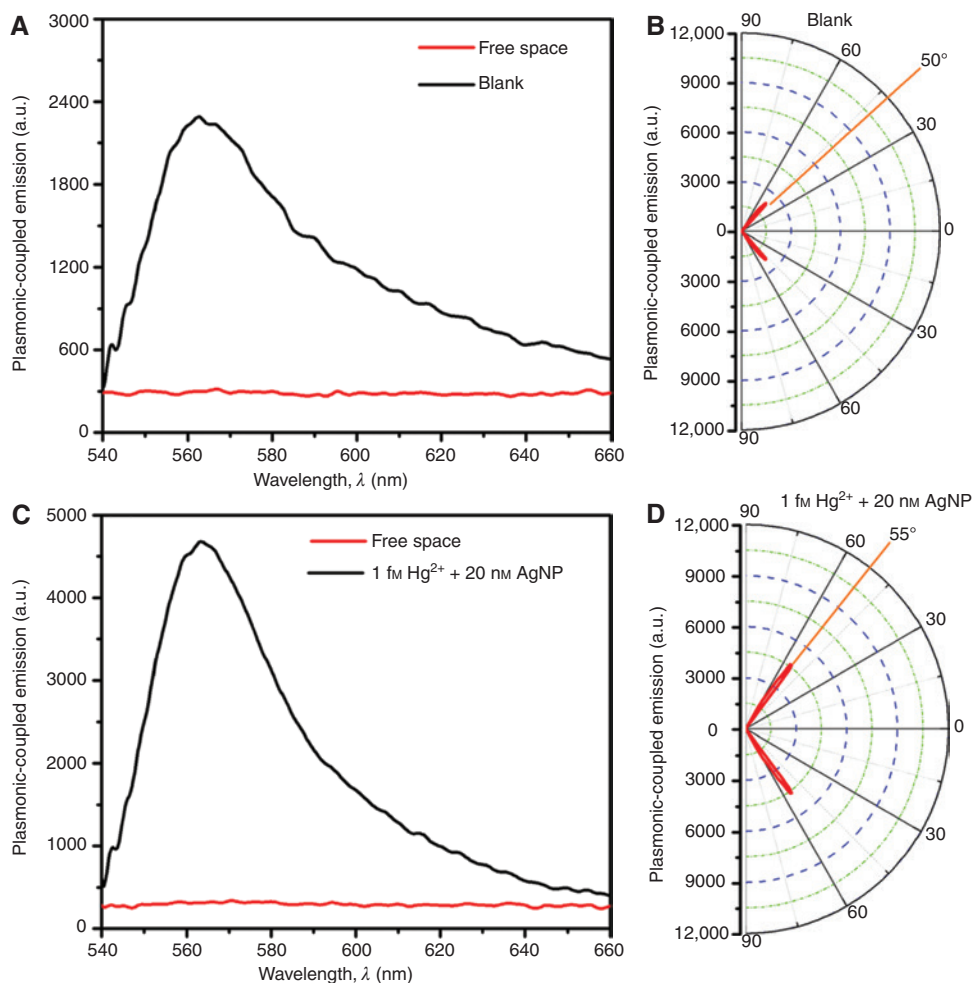

**Figure 5:** In the presence of the AgNP spacer layer, (A) SPCE and FS intensity of Rh6G D in the absence of Hg<sup>2+</sup>; (C) SPCE and FS intensity of Rh6G D in the presence of Hg<sup>2+</sup>; and SPCE radial plots for (B) blank and (D) 1 fM Hg<sup>2+</sup>.

emission at 48°. Figure 3C shows the fluorescence spectrum of Rh6G D in the presence of Hg<sup>2+</sup> (1 pM) along with its FS spectrum, and its SPCE angularity (45°) has been plotted in Figure 3D.

In the second set of experiments, an LOD of 1 fM for Hg<sup>2+</sup> ions was achieved with the use of an AgNP spacer layer. The effect of AgNPs on the coupling efficiency of the radiating dipole with the surface plasmons has been well understood in earlier reports [33, 36]. In the current study, 20 nm AgNPs in 1% PVA were used as the spacer layer. Spacer engineering resulted in amplification of the SPCE enhancements as well as improved sensitivity for Hg<sup>2+</sup> detection. The enhancements in the SPCE signal for both sets of experiments have been tabulated (Table 1). The SPCE enhancements for different concentrations of Hg<sup>2+</sup> ranging from 100 nM to 1 fM in the presence of AgNPs have been plotted in Figure 4. The two slopes in this figure have been obtained for Hg<sup>2+</sup> concentrations in two different ranges: lower (1 fM–1 pM) and higher (10 pM–100 nM). This particular occurrence is not uncommon, as it has already been reported in earlier studies pertaining to mercury determination with the use of glucose biosensors [37]. Figure 5A (blank) and Figure 5C (1 fM Hg<sup>2+</sup>) present the fluorescence intensity plots obtained in the presence of the AgNP spacer. Figure 5B and D present the radial plots for blank and 1 fM concentration of Hg<sup>2+</sup>. Further, the emission was significantly p-polarized in the SPCE region, 95% in the absence and 97% in the presence of AgNPs.

However, the localized surface plasmon resonance of the AgNPs (distributed uniformly throughout the sample matrix) helps in the effective coupling of photons from the radiating dipole with the silver thin film. This results in ultra-amplification of the fluorescence emission and significantly alters the LOD of Hg<sup>2+</sup> ions as seen from the second set of experiments. Currently, studies are under way to analyze multiple analytes (contaminants) in water for comprehensive water quality monitoring, to be achieved with this plasmonic device.

## 4 Conclusions

Rapid and sensitive detection of mercury ions has a great impact on the management of community health and the environment on account of its ubiquitous presence and high toxicity. However, current fluorescence-based technologies have their limitations in sensitivity on account of poor signal collection efficiency. The use of the SPCE platform and an engineered sensor chip (spacer layer) in this context has significantly aided in the achievement of

enhanced sensitivity, resulting in femtomolar detection of Hg<sup>2+</sup>. The ability of AgNPs to increase the coupling efficiency of the fluorophore was utilized to achieve fluorescence enhancements in excess of 80-fold. We are in the process of prototyping a multi-analyte sensing portable device for rapid, low-cost online water monitoring and, in turn, realize an integrated water management approach.

**Acknowledgment:** S.S.R., P.K.B., and V.S. acknowledge the support from DBT Ramalingaswamy fellowship (102/IFD/SAN/776/2015-16), DST Fast Track scheme (no. SR/FT/CS-51/2010(G)) and UGC-BSR fellowship, Government of India. Guidance from Bhagawan Sri Sathya Sai Baba is also gratefully acknowledged.

**Conflict of interest:** The authors declare no conflict of interest.

**Supplementary data:** The following is the supplementary data related to this article: additional information concerning the SPCE measurements and results are available as Supporting Information (SI).

## References

- [1] De Silva AP, Gunaratne HQN, Gunnlaugsson T, Huxley AJM, McCoy CP, Rademacher JT, Rice TE. Signaling recognition events with fluorescent sensors and switches. *Chem. Rev.* 1997, 97, 1515–1566.
- [2] Peng X, Du J, Fan J, Wang J, Wu Y, Zhao J, Sun S, Xu T. A selective fluorescent sensor for imaging Cd<sup>2+</sup> in living cells. *J. Am. Chem. Soc.* 2007, 129, 1500–1501.
- [3] Royzen M, Dai Z, Cannry JW. Ratiometric displacement approach to Cu (II) sensing by fluorescence. *J. Am. Chem. Soc.* 2005, 127, 1612–1613.
- [4] Malm O. Gold mining as a source of mercury exposure in the Brazilian Amazon. *Environ. Res.* 1998, 77, 73–78.
- [5] Nolan EM, Lippard SL. Turn-on and ratiometric mercury sensing in water with a red-emitting probe. *J. Am. Chem. Soc.* 2007, 129, 5910–5918.
- [6] Renzoni A, Zino F. Mercury levels along the food chain and risk for exposed populations. *Environ. Res.* 1998, 77, 68–72.
- [7] Gil DB, Rodriguez-Cáceres MI, Hurtado-Sánchez MC, Pena AM. Fluorescent determination of Hg<sup>2+</sup> in water and fish samples using a chemodosimeter based in a rhodamine 6G derivative and a portable fiber-optic spectrofluorimeter. *Appl. Spectrosc.* 2010, 64, 520–527.
- [8] Sánchez Uria JE, Sanz-Medel A. Inorganic and methylmercury speciation in environmental samples. *Talanta* 1998, 47, 509–524.
- [9] Morita M, Yoshinaga J, Edmonds JS. The determination of mercury species in environmental and biological samples. *Pure Appl. Chem.* 1998, 70, 1585–1615.
- [10] Ncube P, Krause RW, Ndinteh DT, Mamba BB. Fluorescent sensing and determination of mercury (II) ions in water. *Water SA.* 2014, 40, 175–182.

- [11] Shi W, Ma H. Rhodamine B thiolactone: a simple chemosensor for Hg<sup>2+</sup> in aqueous media. *Chem. Commun.* 2008, 16, 1856–1858.
- [12] Zheng H, Qian ZH, Xu L, Yuan FF, Lan LD, Xu JG. Switching the recognition preference of rhodamine B spirolactam by replacing one atom: design of rhodamine B thiohydrazide for recognition of Hg(II) in aqueous solution. *Org. Lett.* 2006, 8, 859–861.
- [13] Kim HN, Nam SW, Swamy KMK, Yan J, Chen X, Kim Y, Kim SJ, Park S, Yoon J. Rhodamine hydrazone derivatives as Hg<sup>2+</sup> selective fluorescent and colorimetric chemosensors and their applications to bio-imaging and microfluidic system. *Analyst* 2011, 136, 1339–1343.
- [14] Pena AM, Rodríguez-Caceres MI, Hurtado-Sanchez MC, Gil DB. A novel application of Hg<sup>2+</sup> based in a spirocyclic rhodamine 6G phenyl-thiosemicarbazide derivative. *Luminiscence* 2010, 25, 229–230.
- [15] Lee SO, An KL, Shin SR, Jun K, Lee JY, Hwang JY, Son Y. Synthesis of rhodamine-based chemosensor and determination of spectral properties. *Mol. Cryst. Liq. Cryst.* 2014, 604, 193–201.
- [16] Nolan EM, Lippard SJ. A “turn-on” fluorescent sensor for the selective detection of mercuric ion in aqueous media. *J. Am. Chem. Soc.* 2003, 125, 14270–14271.
- [17] Nolan EM, Racine ME, Lippard SJ. Selective Hg (II) detection in aqueous solution with thiol derivatized fluoresceins. *Inorg. Chem.* 2006, 45, 2742–2749.
- [18] Kim HJ, Park JE, Choi MG, Ahn S, Chang SK. Selective chromogenic and fluorogenic signaling of Hg<sup>2+</sup> ions using a fluorescein-coumarin conjugate. *Dyes Pigm.* 2010, 84, 54–58.
- [19] Jin Y, Yoon I, Seo J, Lee JE, Moon ST, Kim J, Han SW, Park KM, Lindoy LF, Lee SS. Cadmium(II) and mercury(II) complexes of an NO<sub>2</sub>S<sub>2</sub>-donor macrocycle and its ditopic xylyl-bridged analogue. *Dalton Trans.* 2005, 4, 788–796.
- [20] Wang J, Qian X. Two regioisomeric and exclusively selective Hg(II) sensor molecules composed of a naphthalimide fluorophore and an O-phenylenediamine derived triamide receptor. *Chem. Commun.* 2006, 1, 109–111.
- [21] Tang CX, Zhao Y, He XW, Yin XB. A ‘turn-on’ electro-chemiluminescent biosensor for detecting Hg<sup>2+</sup> at femtomole level based on the intercalation of Ru(phen)<sub>3</sub><sup>2+</sup> into ds-DNA. *Chem. Commun.* 2010, 46, 9022–9024.
- [22] Virta M, Lampinen J, Karp M. A luminescence-based mercury biosensor. *Anal. Chem.* 1995, 67, 667–669.
- [23] Xue X, Wang F, Liu X. One-step, room temperature, colorimetric detection of mercury (Hg<sup>2+</sup>) using DNA/nanoparticle conjugates. *J. Am. Chem. Soc.* 2008, 130, 3244–3245.
- [24] Zhao Y, Zhong Z. Tuning the sensitivity of a foldamer based mercury sensor by its folding energy. *J. Am. Chem. Soc.* 2006, 128, 9988–9989.
- [25] Vannela R, Adriaens P. In vitro selection of Hg (II) and As (V)-dependent RNA-cleaving DNazymes. *Environ. Eng. Sci.* 2007, 24, 73–84.
- [26] Lakowicz JR. Radiative decay engineering-3 surface plasmon-coupled directional emission. *Anal. Biochem.* 2004, 324, 153–169.
- [27] Yoon H, Maier SA, Bradley DD, Stavrinou PN. Surface plasmon coupled emission using conjugated light-emitting polymer films. *Opt. Mater. Express* 2011, 1, 1127–1138.
- [28] Srinivasan V, Badiya PK, Ramamurthy SS. Low-dimensional carbon spacers in surface plasmon-coupled emission with femtomolar sensitivity and 1000-fold fluorescence enhancements. *Chem. Commun.* 2015, 51, 7809–7811.
- [29] Srinivasan V, Vernekar DV, Jaiswal G, Jagadeesan D, Ramamurthy SS. Earth abundant iron-rich N-doped graphene based spacer and cavity materials for surface plasmon-coupled emission enhancements. *ACS Appl. Mater. Interfaces* 2016, 8, 12324–12329.
- [30] Srinivasan V, Badiya PK, Ramamurthy SS. Purcell factor based understanding of enhancements in surface plasmon-coupled emission with DNA architectures. *Phys. Chem. Chem. Phys.* 2016, 18, 681–684.
- [31] Srinivasan V, Ramamurthy SS. Purcell factor: a tunable metric for plasmon-coupled fluorescence emission enhancements in cermet nanocavities. *J. Phys. Chem. C* 2015, 120, 2908–2913.
- [32] Badiya PK, Srinivasan V, Jayakumar TP, Ramamurthy SS. Ag-CNT architectures for attomolar dopamine detection and 100-fold fluorescence enhancements with cellphone-based surface plasmon-coupled emission platform. *ChemPhysChem* 2016, 17, 2791–2794.
- [33] Srinivasan V, Ghajesh S, Ramamurthy SS. 1-Minute spacer layer engineering for tunable enhancements in surface plasmon-coupled emission. *Plasmonics* 2015, 10, 489–494.
- [34] Srinivasan V, Kumar MA, Patnaik SG, Ramamurthy SS. Cell-phone monitoring of multi-qubit decay in tunable coupling regimes with attomolar sensitivity. *ACS Appl. Mater. Interfaces* 2016, 8, 23281–23288.
- [35] Brasca R, Onaindia MC, Goicoechea HC, Peña AM, Culzoni MJ. Highly selective and ultrasensitive turn-on luminescence chemosensor for mercury (II) determination based on the rhodamine 6G derivative FC1 and Au nanoparticles. *Sensors* 2016, 16, 1652–1612.
- [36] Chowdhury MH, Ray K, Geddes CD, Lakowicz JR. Use of silver nanoparticles to enhance surface plasmon-coupled emission (SPCE). *Chem. Phys. Lett.* 2008, 452, 162–167.
- [37] Liu J, Xu X, Tang L, Zeng G. Determination of trace mercury in compost extract by inhibition based glucose oxidase biosensor. *Trans. Nonferrous Met. Soc. China* 2009, 19, 235–240.

**Supplemental Material:** The online version of this article (DOI: 10.1515/ntrev-2017-0124) offers supplementary material, available to authorized users.

## Bionotes



**Pradeep Kumar Badiya**

Plasmonics Laboratory, Department of Chemistry, Sri Sathya Sai Institute of Higher Learning, Prasanthi Nilayam, Anantapur, Andhra Pradesh 515134, India

Pradeep Kumar Badiya is a doctoral research scholar (Basic Scientific Research fellow, UGC, India) at the Department of Chemistry, Sri Sathya Sai Institute of Higher Learning. He had completed his MSc and MPhil in chemistry. His current research interests include the bio-processing and fermentation and synthesis of low-cost nanomaterials and thin films for biomedical applications using agricultural biomass.





**Tejkiran Pindi Jayakumar**  
Plasmonics Laboratory, Department of  
Chemistry, Sri Sathya Sai Institute of Higher  
Learning, Prasanthi Nilayam, Anantapur,  
Andhra Pradesh 515134, India

Tejkiran Pindi Jayakumar completed his Master of Science in chemistry at Sri Sathya Sai Institute of Higher Learning. Currently, he is a post-masters researcher at Matsumi Laboratory in School of Materials Science, Japan Advanced Institute of Science and Technology, Japan. His current research interests include synthesis of novel and low-cost efficient material for energy storage devices, and synthesis of plasmonic materials for biomedical applications.



**Venkatesh Srinivasan**  
Plasmonics Laboratory, Department of  
Chemistry, Sri Sathya Sai Institute of Higher  
Learning, Prasanthi Nilayam, Anantapur,  
Andhra Pradesh 515134, India

Venkatesh Srinivasan obtained his PhD in chemistry as a Basic Scientific Research fellow (UGC, Government of India) from Sri Sathya Sai Institute of Higher Learning. He received Master of Science and Master of Philosophy degrees in chemistry from the same institution. He was recognized as Young Scientist 2016 in Physics by Dr. K. V. Rao Scientific Society, Hyderabad, India, for his research on mobile-based plasmonics technology. Currently, he is a research associate at the University of Maryland, Baltimore County, USA, focusing on the development of plasmonic sensors, light-matter interactions, and nanophotonics.



**Sai Sathish Ramamurthy**  
Plasmonics Laboratory, Department of  
Chemistry, Sri Sathya Sai Institute of Higher  
Learning, Prasanthi Nilayam, Anantapur,  
Andhra Pradesh 515134, India,  
Phone: +91-8790314405,  
[rsaisathish@sssihl.edu.in](mailto:rsaisathish@sssihl.edu.in)

Sai Sathish Ramamurthy is currently an assistant professor at the Department of Chemistry, Sri Sathya Sai Institute of Higher Learning (SSSIHL). He was awarded the prestigious Ramalingaswami Fellowship by the Department of Biotechnology, Government of India, in 2011. On receiving his PhD in analytical chemistry from SSSIHL in 2007, Dr. Ramamurthy served as research assistant professor at Center for Advanced Sensor Technology, University of Maryland Baltimore County, USA. On return to his alma mater, he initiated research on the use of the surface plasmon-coupled emission platform at the Plasmonics Laboratory of SSSIHL. He envisions an integrated approach for pursuing translational research in environment, health, and energy with the use of electrochemistry, plasmonics, and bioprocessing techniques. Dr. Ramamurthy has to his credit over 60 publications in book chapters, and national and international peer-reviewed journals.